


erbe
power your performance.

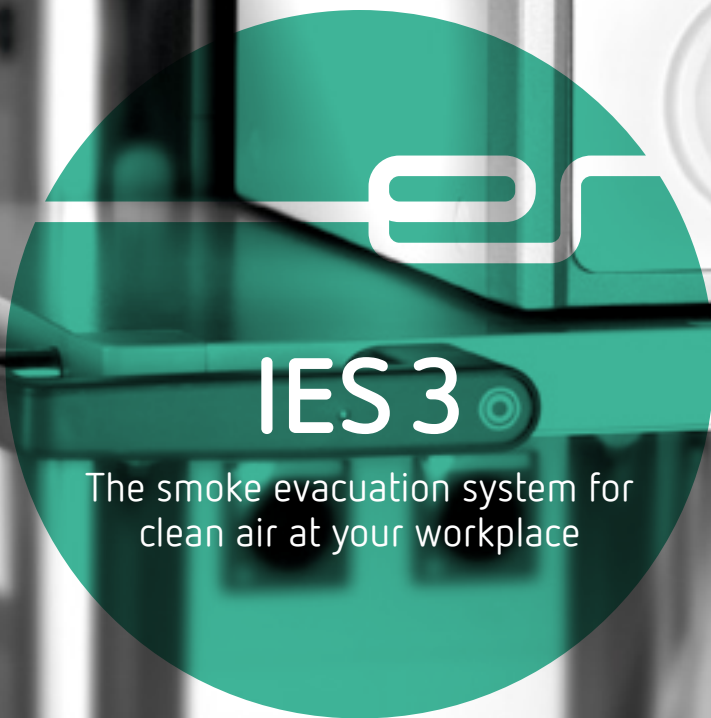

IES 3 smoke evacu

Our solution for a safe working environment

Eliminate surgical smoke with all its potentially dangerous substances from operating rooms, outpatient facilities and medical practices.

Smoke evacuation with IES 3 reduces the smoke concentration in the operating room – and thus also your smoke exposure.^{1,2} A face mask allows too many particles to pass through.^{2,3}

Direct evacuation with an electrosurgical pencil just a few millimeters above the source is more efficient than conventional ventilation systems.⁴ This always gives you a good view of the surgical field and the surgical site itself.³

HAZARD DETECTED. RISK AVERTED. INFORMATION AT: SMOKE.ERBE-MED.COM


Protection through ULPA-15 filter

One core component of the 5-stage main filter cartridge is the ULPA-15 filter which removes 99.9995 % of all 0.1 µm particles.⁵ It offers the best possible safety.^{3,4} The active carbon barrier in the main filter reduces odors. The display indicates the remaining filter capacity at all times.⁶ Changing the filter is simple and convenient.⁷

The optional prefilter protects the main filter cartridge against penetration of liquids and impurities via coarser tissue particles.

Good response, quiet operation

The innovative bi-turbo technology ensures a clean and safe working environment within a very short time through effective and fast evacuation.⁷ Due to the enhanced noise insulation, the IES 3 is noticeably quieter and more pleasant than comparable devices.⁸

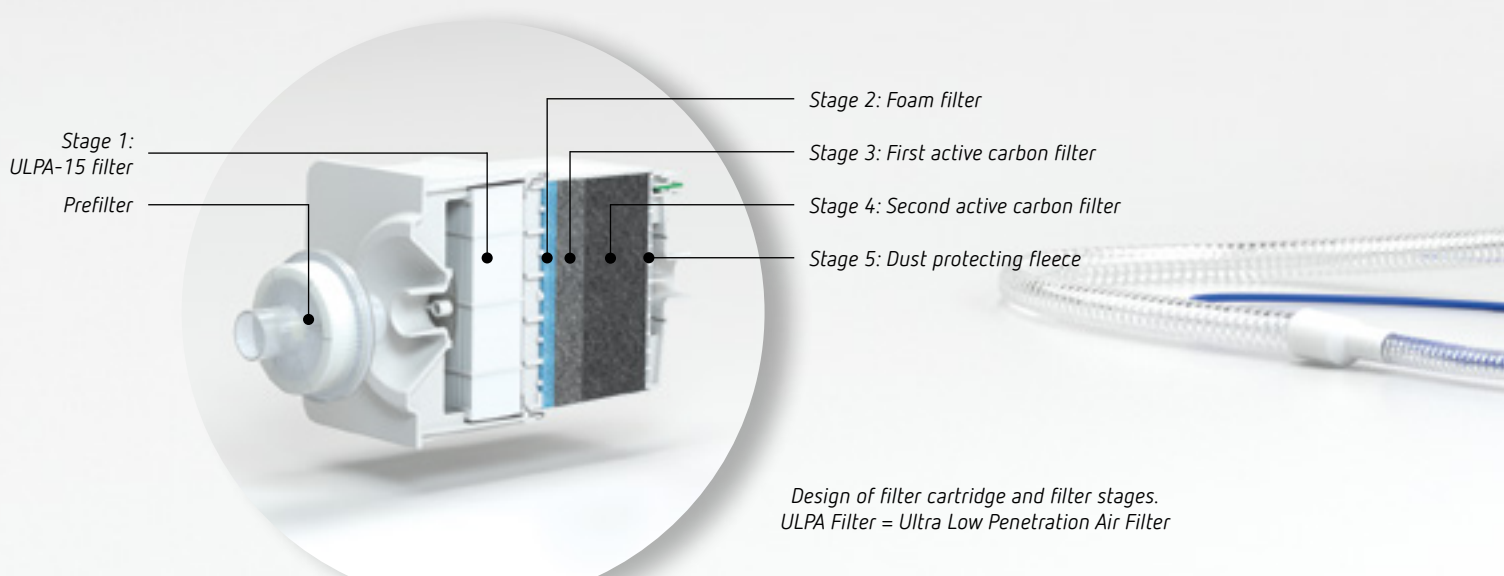

*Design of filter cartridge and filter stages.
ULPA Filter = Ultra Low Penetration Air Filter*

uation system

Extended range of applications

The different operating modes of the IES 3 allow versatile use:

- ☑ Open surgical mode (OPEN Mode)
- ☑ Laparoscopic mode (LAP Mode) with special accessories such as the LAP tubing set with or without trumpet valve (3 m and 5 m)
- ☑ Presettings and configurations allow immediate use for different clinical requirements

Flexible activation

You have the following options for activating the IES 3 individually – regardless of working with one or two instruments simultaneously:

- ☑ Automatically via the VIO® activation
- ☑ Via the automatic activation device for all electro-surgical units
- ☑ Via the foot switch for laser and ultrasonic applications

91 %
OF RESPONDENTS
REGARD THE IES 3
AS QUIET AND
PLEASANT.⁷



Our complete package

Smoke evacuation made by Erbe

Benefit from our almost 100 years of experience in electrosurgery, our worldwide presence and international support. The IES 3 is our contribution to a safe working environment.^{1,3}

90 %
OF ALL
RESPONDENTS
REGARD THE IES 3
USER INTERFACE
AS INTUITIVELY
EASY.⁷



HORIZONTAL



VERTICAL



INTEGRATED IN THE VIO® 3 WORKSTATION

Easy and intuitive to use

- ☑ Compatible with all models of the VIO® range
- ☑ Fast and user-friendly operation:⁷
 - Proven user interface, similar to the VIO® 3 touchscreen
 - Display shows all parameters at a glance (settings, filter runtime, notes for the user)

High flexibility, compact design

- ☑ Smoke evacuation for every surgical discipline
- ☑ In the operating room as well as in outpatient facilities and medical practices
- ☑ For electrosurgery, laser, ultrasound
- ☑ Can be integrated into the VIO® workstation
- ☑ Can be used as stand-alone device
- ☑ Can be positioned horizontally or vertically

A system with variable configurations – all from one source



The **Water trap and prefilter** protect the high-efficiency filter.



The **connection to the central evacuation system** removes particles and odors from the operating field.



The **automatic activation device** enables starting the IES 3 with all electrosurgical devices.



Good view of the target area in LAP mode with the **LAP tubing set**.



The **T-piece** offers optimal simultaneous evacuation even with 2 instruments.



The **one-pedal footswitch** activates the IES 3 in combination with laser and ultrasonic devices.

The **single-use smoke evacuation pencils** extract surgical smoke directly at its source.



Instruments		
20321-028	Electrosurgical pencil for IES, telescoping with spatula electrode	
20321-040	Smoke evacuation pencil, single-use, short with spatula electrode, connecting cable 3 m	
20321-041	Smoke evacuation pencil, single-use, short with coated spatula electrode, connecting cable 3 m	
20321-042	Smoke evacuation pencil, single-use, short with spatula electrode, connecting cable 5 m	
20321-043	Smoke evacuation pencil, single-use, short with coated spatula electrode, connecting cable 5 m	
20321-044	Clip-On handle for smoke evacuation To be used in combination with Erbe Slim-Line electrosurgical pencils (20190-065, 20190-066, 20190-067, 20190-074, 20190-075)	
20321-045	Extension tip for Clip-On handle To be used in combination with 20321-044	

Technical data

Power connection

Rated supply voltage	100–240V AC ($\pm 10\%$)
Rated supply frequency	50/60 Hz
Line current	max. 3 A
Power consumption	max. 300 watts
Stand-by	12 watts at 230V, 12 watts at 115V
Potential equalization connection	Yes
Power fuse	T 4 A H / 250 V

Type of operation

Continuous operation

Unit data

Filter specifications	ULPA-15 in accordance with EN 1822-3:2011 and EN 1822-5:2011, corresponds to the requirements of ISO 16571 smoke evacuation devices
Noise development	At 60 % evacuation power ≤ 49 dB(A) according to DIN EN ISO 3744 At max. evacuation power ≤ 59 dB(A) according to DIN EN ISO 3744
Extraction performance	≤ 730 l/min (maximum turbine power, th) ≤ 300 l/min (with main filter cartridge, automatic shut-off)

Dimensions and weight

Width x height x depth	205 x 280 x 404 mm
Weight	9.7 kg including main filter cartridge
Display size	5.7 inches

Ambient conditions for operating the unit

Temperature	+10 °C to +40 °C
Relative humidity	15 %–85 %, non-condensing
Air pressure	54 kPa–106 kPa
Max. operating height	5000 m over SL

Acclimatization

If the unit has been stored or transported at temperatures below +10 °C or above +40 °C, the unit will take approximately 3 hours to acclimatize to room temperature.

Standards

Classification in accordance with MDD 93/42 EEC	I
Protection class in accordance with EN 60 601-1	I
Type in accordance with EN 60 601-1	CF

Smoke evacuation system and accessories

Smoke evacuation system consisting of:

10323-000	IES 3 smoke evacuation unit
20323-000	Main filter cartridge IES 3

Accessories for protecting the main filter cartridge

20321-022	Prefilter for smoke evacuation
20323-004	Self-sealing water trap; right angled, medium volume

Accessories for laparoscopic application and simultaneous application

20323-003	LAP tubing set IES 3 with trumpet valve 3 m
20323-006	LAP tubing set IES 3 with trumpet valve 5 m
20323-010	LAP tubing set IES 3 without valve 5 m
20323-011	LAP tubing set IES 3 without valve 5 m
20323-005	T-piece 22 mm outer diameter, 22 mm inner diameter, 22 mm outer diameter

Accessories for open surgical application

20321-004	Evacuation tube with optimized streaming
20321-009	Evacuation tubing, ø 22 mm
20321-010	Evacuation funnel connection, ø 22 mm
20321-012	Evacuation tubing, ø 22 mm, length 2.1 m (reusable)

Accessories for connection to central evacuation system

20323-001	Evacuation element IES 3 for central evacuation
20323-009	Smoke evacuation tubing, ø 32 mm, length 1.8 m, type VT 10106

Attachment sets

20180-132	Attachment set IES 2 / IES 3 to VIO® CART 20180-000
20323-008	Attachment set VIO® C to IES 3
20323-007	Attachment set IES 3 to VIO® 3

Accessories for activation options

20323-002	Automatic activation device for IES 3 for VIO® C, electrosurgical external devices or stand-alone operation
20322-101	One-pedal footswitch IES 2 / IES 3 AP & IP X8 equipment

References

- 1 Schultz L: Can efficient smoke evacuation limit aerosolization of bacteria? *AORN J.* 2015 Jul; 102(1):7-14.
- 2 R S Parsa, N J Dirig, I N Eck, W K Payne III.: *Surgical Smoke and the Orthopedic Implications. The Internet Journal of Orthopedic Surgery.* 2015 Volume 24 Number 1
- 3 BRENDA C. ULMER, RN, MN, CNOR: *The Hazards of Surgical Smoke; AORN J.* 2008, Vol 87, No. 4: 721-734.
- 4 Karsai S et al: *Smoking guns: hazards generated by laser and electrocautery smoke. J Dtsch Dermatol Ges.* 2012 Sep;10(9): 633-6.
- 5 Internal data: VB_Filter qualification ULPA15 IES 3; D158650
- 6 Internal data: filter service life IES 3; D138347
- 7 Internal data: results of summary evaluation II; D158302
- 8 Internal data: VB_sound measurements IES 3; D162979

Important information

The information, recommendations and other details contained in this medium ("information") reflect our state of knowledge and the state of the art in science and technology at the time the medium was created. The information is of a general nature, non-binding and intended solely for general information purposes; it does not constitute instructions for use.

The information and recommendations contained in this medium do not create any legal obligations on the part of Erbe Elektromedizin GmbH and its affiliated companies ("Erbe") or any other claims against Erbe. The information does not constitute any guarantees or other information on the nature of the product; such information requires an express contractual agreement with Erbe in each individual case.

Erbe is not liable for any kind of damage resulting from following the information on this medium, regardless of any legal grounds for liability.

Every user of an Erbe product is responsible for testing the respective Erbe product in advance with regard to its properties and its suitability for the intended type of use or purpose. Suitable type of use of the respective Erbe product can be found in the instructions for use for the respective Erbe product. The user is obliged to ascertain whether the instructions for use available to him/her correspond to the current status of the specific Erbe product. Devices may only be used in accordance with the instructions for use.

Information on settings, application sites, application duration and use of the respective Erbe product is based on the clinical experience of individual centers, physicians and clinical literature independent of Erbe as well as post market surveillance and empirical evidence. They constitute reference values, or Experienced Starting Settings, which must be checked by the user to ensure that they are suitable for the specifically planned application. Depending on the circumstances of a specific application, it may be necessary to deviate from the information provided. The user is responsible for checking this when using Erbe products. We wish to note that science and technology are subject to constant development as a result of research and clinical experience. Similarly, medicine and clinical application are constantly evolving as a result of research and technological development. This may also make it necessary for the user to deviate from the information provided on this medium.

This medium contains information about Erbe products that may not be approved/cleared in certain countries. The user of the respective Erbe product is obliged to inform himself/herself as to whether the Erbe product he/she is using is legally approved/cleared in his/her country and/or to what extent, if any, there are legal requirements for or restrictions on its use.

This medium is not intended for use in the USA.

Erbe Elektromedizin GmbH
Waldhoernlestrasse 17
72072 Tuebingen
Germany

Phone +49 7071 755-0
info@erbe-med.com
erbe-med.com
medical-videos.com